

## Protocol for Real-Time RT-PCR SARS-CoV-2 (2019-nCoV) (E gene) with P&P

**For RUO (Research Use Only)**

**Caution:** The vials containing the primers and probe mix (P&P) should be stored after reception at -20°C in the dark. Stable at least 6 months in the described conditions.

NB: Probe: FAM-QSY

Reagents with which the assay has been validated at UVE (Unité des Virus Emergents, Marseille, France):

- SuperScript™ III Platinum™ One-Step qRT-PCR Kit , ThermoFischer ref 11732-088
- Elution Buffer AE (1000 ml) Macherey-Nagel™ ref 740917.1 (This component is not provided with the OneStep RT-PCR kit); usually provided as elution buffer in the extraction kit, (10mM TrisHCl 0.5mM EDTA, pH=9).

### 1. Rehydration of Lyoph-P&P before use (Table 1)

- Write the date on the vial before opening.
- Lyoph-P&P is resuspended as described:
  - Add 182 µl of AE Elution buffer
  - Homogenization by 10 to 20 times pipetting up and down in the glass vial a 50µL-volume
  - Rehydrated P&P must be incubated at room temperature for 10 min after which
  - A second step of 10 times multiple pipetting must be done.

**WARNING: These steps are critical to ensure adequate homogenization**

**Table 1. Lyoph-P&P regeneration; rehydrated Lyoph-P&P can be stored at 4 °C for up to 14 days**

Number of tests/vial	24
AE Elution buffer (µL)	182*

**\* this volume is adapted to the SuperScript™ III Platinum™ One-Step qRT-PCR Kit and can vary depending upon the RT-PCR kit**

## 2. Preparation of the reaction MIX

MasterMix	25 $\mu$ L Single rxn, $\mu$ L
2X Reaction mix*	12.5
Rehydrated Primers and probe P&P**	7.0
SSIII/Taq EnzymeMix*	0.5
	20
Template RNA	5

\* , ThermoFischer / Invitrogen: SuperscriptIII One-Step RT-PCR system with Platinum Taq DNA Polymerase

\*\*, as indicated in Table 1.

## 3. Cycling program and RT-PCR reaction

- 1: 50°C for 15 min
- 2: 95°C for 2 min
- 3: 95°C for 15 sec
- 4: 58°C for 45 sec
- Plate Read
- 5: GOTO 3, 44 more times

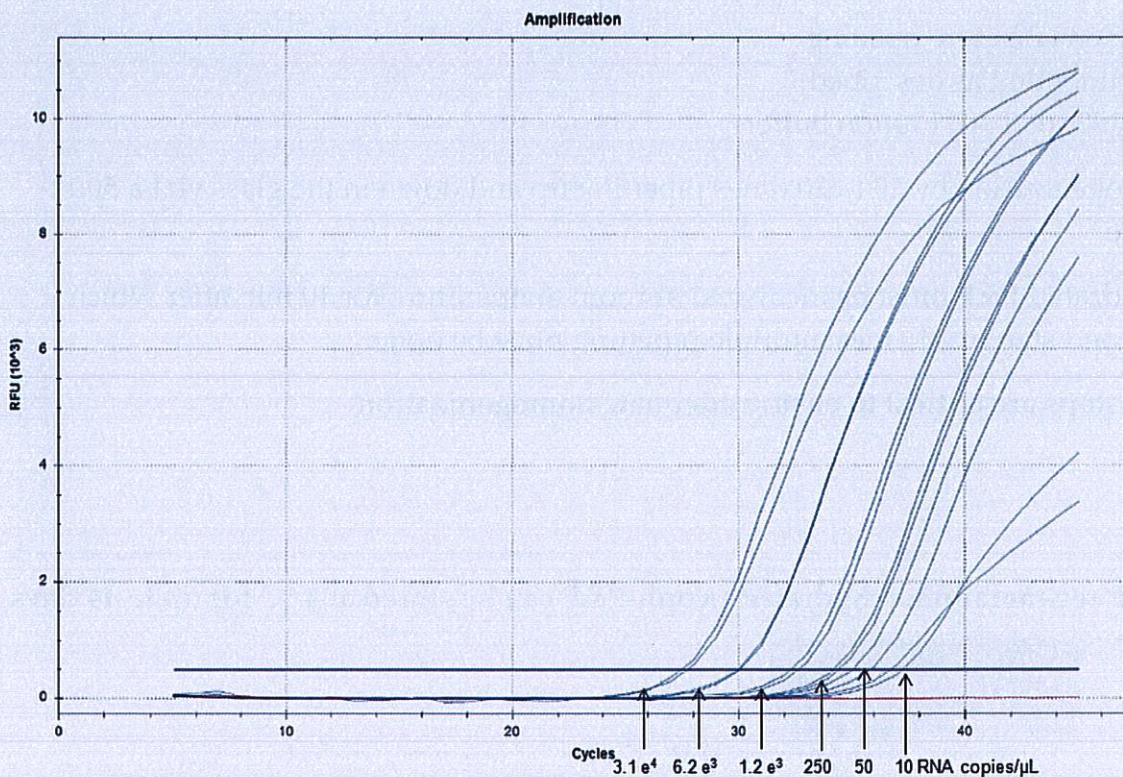


Figure. Results obtained with 5-fold serial dilutions of 2019-nCoV E gene encapsidated RNA.



National Institute for Public Health  
and the Environment  
Ministry of Health, Welfare and Sport

## CERTIFICATE OF PARTICIPATION

awarded to

**Unité des virus émergents,  
Aix-Marseille University, France**

to attest completion of ERLI-Net & EVD-LabNet

## EXTERNAL QUALITY ASSESSMENT SCHEME FOR

## MOLECULAR DIAGNOSTICS OF SARS-CoV-2, JULY 2020

Covering the following:

- Accurate detection of SARS-CoV-2 in 12 coded and inactivated samples

Organised by:

**European Centre for Disease Prevention and Control**  
Mike Catchpole, Chief Scientist

Performed under ECDC/2017/002 specific contract 3 by:  
**National Institute for Public Health and the Environment – The Netherlands (RIVM)**  
Chantal Reusken, coordinator EQA and EVD-LabNet

**Charité – Berlin (CUB)**  
Jan Felix Drexler, coordinator EQA

